


Wipe Test Results

Biodex Model 086-332 Serial # 08070015 Detector Serial # 9020011

04/27/2009 13:15
Test Date

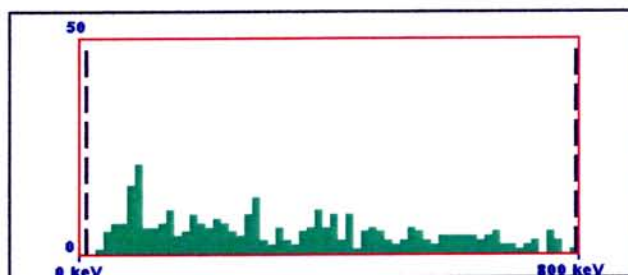

Highlighted ROI: Wide Window

Full Spectrum

Net Cnts: -10
Total Net CPM: -10.0
Test Time (secs): 60
Net Cnts>800keV: -14

Wide Window

Total Efficiency: 34.47%
Background: 908 DPM
Net Activity: 12 DPM
Net CPM: 4.0
ROI: 25 - 800 keV
Trigger Level: 20,000 DPM

Location: Hot Lab

Technologist: AMA

Status: **PASS - Acceptable Level**

	<u>Isotope</u>	<u>Background</u>	<u>Net Activity</u>	<u>Net CPM</u>	<u>Trigger</u>	<u>Status</u>
1	Ga-67	422 DPM	-8 DPM	-4.0	20,000 DPM	PASS
2	I-131	153 DPM	-8 DPM	-3.0	2,000 DPM	PASS
3	Tc-99m	41 DPM	0 DPM	0.0	20,000 DPM	PASS
4	Tl-201	131 DPM	-16 DPM	-8.0	20,000 DPM	PASS

Approved By: _____

Date: _____